


Fitting Instructions

OA Knee Sleeve X1

Model: 11005 & 11006 Size: S/M/L/XL/XXL

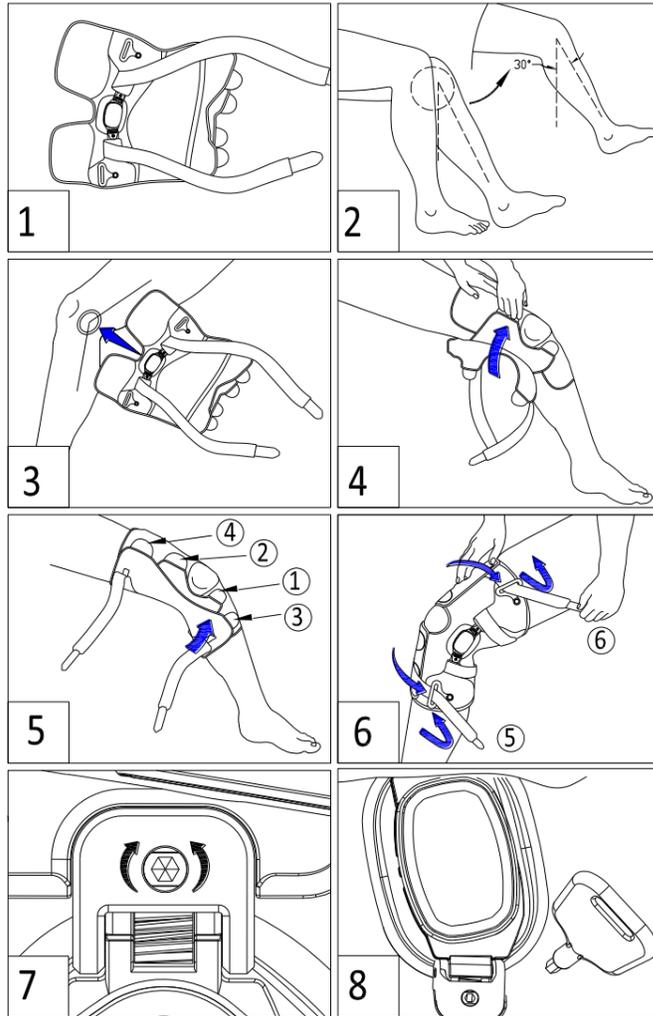

APPLICATION INSTRUCTIONS:

NOTICE: Before use, please set the hinge of 0 ° on horizontal position. The setting of the support angle should be performed by a trained professional in accordance with the doctor's instructions for inner and outer unloading, which will be adjusted in step 5.

STEP 1. Untie two straps and open the brace. Knee bends 30 °, align the position of the hinge center and the center of the knee alignment, and then hold in place to prevent slide (figure 1~3). **STEP 2.** Pull the four pieces over the knees and legs in turn 1-2-3-4 and fasten them firmly (Fig .4~5).

STEP 3. Pull the calf strap #5 through the buckle and tie it tight. Repeat thigh strap #6 (fig.6).

STEP 4. With the knee bent to 30 degrees, on both the upper and lower hinge screw turn anti-clockwise by 1/8 turn with the adjustment tool to increase unloading on the outer side (opposite side to the hinges). This is the best starting point for initial use.

STEP 4-1. Stand and walk short distances to ensure comfort after each adjustment. If there is any discomfort to the knee or leg adjust the angle back slightly. If more unloading is required turn the hinge screws no more than 1/8 turn in anti clockwise direction. Walk after adjustment and check for comfort

*IMPORTANT:

Excessive adjustment of hinge center screws may cause discomfort or skin pressure problems. Please adjust carefully

"WEARING TIME" :

Gradually increase the wearing time of the Brace and adjust the wearing time of the brace if your body allows.

PREOPERATIVE WEARING TIME:

The first wearing time starts from 30 minutes and gradually increases to no less than 2 hours per day according to the degree of body adaptation. The supporting angle of hinge can be adjusted again in condition of no discomfort.

POSTOPERATIVE WEARING:


The standard of wearing should be decided by the doctor, including the angle of hinge support, the angle of flexion and extension, and the time of wearing every day. The pain caused by osteoarthritis takes time to subside. Wearing a brace regularly for weight-bearing activities (such as walking) will start to feel lighter as it will reduce joint load. This may require wearing it for weeks or even more time to reduce joint load until your primary care physician allows you to remove the brace.

RANGE OF MOTION ADJUSTMENTS

Start from the standard 0 °, additional flexion and extension angle accessories can be installed and they shall be fitted by the doctor as required.

Optional extension angles include 5°, 10°, 15°, 20°, and 25°; Optional flexion angles include 30°, 45°, 60°, 75°, and 90°.

*Please purchase and use the product under the guidance of your doctor or professional.

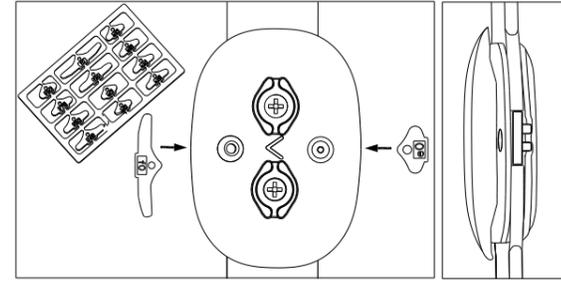

CARE AND MAINTENANCE

High elastic fabric body can use neutral detergent and 30 °C water washing by hand, and natural dry. Do not use clothe dryer or other heat source for drying.

Metal parts should not be washed with water. Hinges can be lubricated with dry silicone spray.

WARNINGS:

If you experience pain, swelling, sensory changes, or discomfort with this product, please stop using and contact your doctor.

FOR SINGLE PATIENT USE ONLY

NOTICE: The device is a one-element holistic treatment program managed by medical professionals. There is no guarantee that damage can be prevented by using the device.

BASIC PRODUCT ENVIRONMENT

- 1) Ambient temperature: -15 ~ 60°C
- 2) Relative humidity: ≤80%

PRODUCT MATERIALS

- 1) High elastic fabric body: spandex fiber
- 2) Metal support: aluminum alloy/stainless steel
- 3) Buckle: nylon
- 4) Angle adjusting key: nylon/carbon steel
- 5) Strap: nylon/polyurethane/polyester

CONTRAINDICATION

- Use with caution for unstable fractures;
- Use with caution in osteoporosis;
- Use with caution for cognitive impairment;
- Use with caution for bony ankylosis;

STORAGE, TRANSPORTATION AND EXPIRY DATE OF PRODUCTS

- 1) Term of validity: 5 years.
- 2) Storage of the product: please put it in a dry and clean room before use to ensure indoor ventilation.

3) Transportation: the product shall be dustproof, Moisture-proof and pollution-proof during storage and transportation.

WASTE DISPOSAL

Disposal of wrapping paper (bags): Please dispose of the packaging of this product according to the local laws.

SYMBOL AND PICTURE DESCRIPTION

- Attention, warning
- Hand wash only
- Protect from sunlight
- Do not use when the packing is damaged
- It is valid for five years
- Reference instructions

ACCESSORIES LIST

- Instructions ----- 1 COPY
- Angle adjusting accessories ---- 1 SET
- Angle adjustment key ---- 1PCS
- Hexagon wrench ---- 1PCS
- Knee pad ---- 1 PCS (sets)

AFTER-SALES WARRANTY

Warranty: all products from the date of purchase as the original date, normal wear and tear of the product in the use of the process is not considered defective.

The following parts from the date of purchase to the warranty period, if there is any material or process defects, please contact your seller directly, simple medical will complete or partial repair or replacement of equipment and accessories.

Metal support ---- 1 year

Distributed by: Promedics Orthopaedic Ltd
Block 7, Gareloch Road
Port Glasgow
PA14 5XH
www.promedics.co.uk



Trademark belongs to Simple Medical (Shenzhen) Limited.

Manufacturer: AC Mould (Dongguan) Limited
No.1 Miya Road, Fenggang Town,
Dongguan City, Guangdong Province,
China.523696 .



Not made with natural rubber latex.

PRODUCT STRUCTURE AND PERFORMANCE

The product is mainly made of high elastic fabric body, metal bracket, straps, key and accessories. Lightweight design with support and soft liner. The unique patented hinge technology can effectively reduce the load of knee varus or valgus. By optimizing the angle adjustment, it helps to relieve the pain and pressure points of the knee joint. The high elastic fabric makes the brace and thigh/calf properly protected, and the special contour design improves the patient's ligament protection and comfort. The product is suitable for a variety of uses, so that patients get a good recovery.

INDICATIONS:


- Mild to severe unicompartmental knee osteoarthritis
- Meniscus procedures/repairs
- Medial or lateral compartment

Fitting Instructions

产品说明书

膝部固定器

产品型号:11005&11006 产品规格:S/M/L/XL/XXL

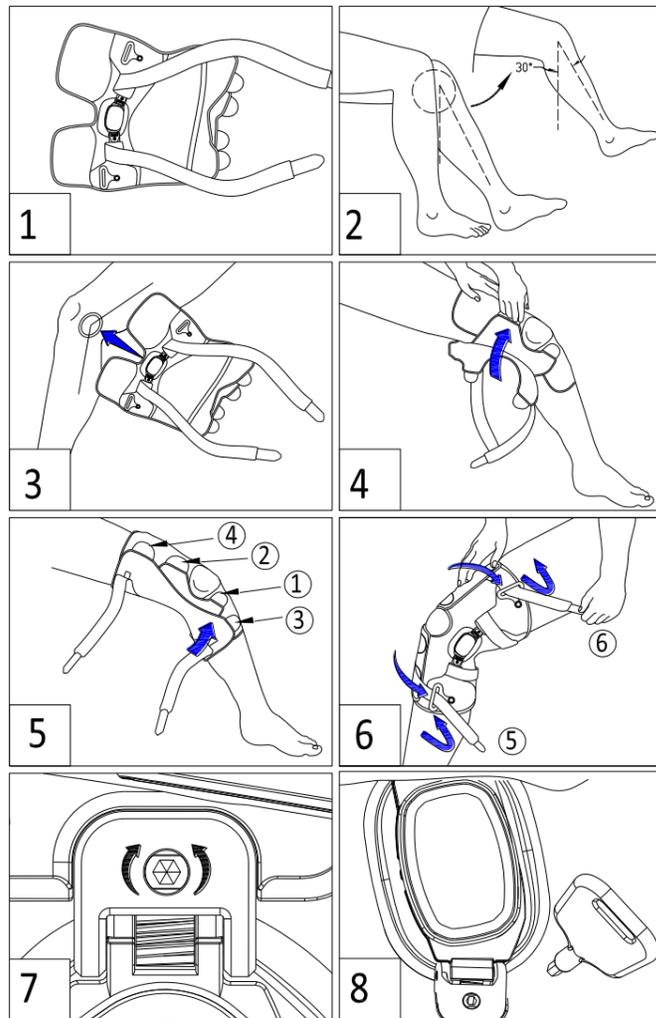

一. 产品结构及性能

支具主要由高弹力面料外套，金属支架，绑带，钥匙及配件等组成。产品采用轻量化的设计，设置有支撑器和软衬垫。通过支撑器的独家专利技术铰链，能够有效减轻膝内翻或外翻的负荷。通过角度调整的优化，有助于缓解膝关节的疼痛和压力点。高弹力面料使得支具与大/小腿有妥帖的保护，特别的轮廓设计，提高了患者的韧带保护性和穿戴舒适度。产品适合多种用途，有效保障患者得到良好的康复。

二. 适应症

- 用于轻度至重度单侧膝骨关节炎
- 半月板术后康复
- 膝关节内外翻

三. 应用说明

警告：在使用之前，请将铰链设置为 0° 即水平位置。设置支撑角应由受过训练的专业人员按照医生的指示进行内外侧卸荷，将在步骤 5 进行调整。

步骤 1：解开两条绑带并打开支具。膝盖弯曲 30° 使铰链中心位置与膝盖中心位置对齐并用手固定住(图 1~3)。

步骤 2：将 4 个拉片依次按 1-2-3-4 拉过膝盖和大小腿处，并牢牢地紧固(图 4~5)。

步骤 3：将小腿绑带#5 穿过绑带扣并系紧。重复大腿绑带#6(图 6)。

步骤 4：支撑的初始安装：膝盖弯曲 90°，用调整工具把铰链中心螺丝顺时针转动 1/8 圈（重要）增加外侧面的卸荷或逆时针 1/8 圈向中心卸荷。这是初次使用的最佳起点(图 7~8)。

步骤 4.1：站立和行走短距离，以确保每次调整和校正支撑后的舒适度。如果膝关节或腿部有任何不适，请稍微向后调整角度。

如果需要更多的卸荷可拧铰链中心螺丝不超过 1 / 8 圈，在调整后行走并检查舒适度。

***重要事项：过度调整铰链中心螺丝可能引起不适或皮肤压力问题。请谨慎调整。**

“穿戴时间”：

逐渐增加支架的穿戴时间。在身体允许的状态下调整支具的穿戴时间。

术前穿戴时间：第一次穿戴时间由 30 分钟开始，根据身体的适应程度，逐渐增加到每天不少于 2 小时的穿戴时间，在身体没有不适的情况下再调整铰链的支撑角度。


术后穿戴：支具穿戴标准应由医生来制定铰链支撑的角度和屈伸的角度以及每天的穿戴时间。

骨关节炎引起的疼痛需要时间来消退。经常穿戴支具负重活动（例如：步行），会让你开始感觉轻松，因为它会减轻关节负荷。这可能需要佩戴几个星期或以上来减轻关节负荷，直至你的主治医生同意你取下支具。

运动调整范围：

支撑从标准 0° 延伸。可以安装额外的屈伸/延长角度，他们是由医生按规定或需要来安装适合的支撑角度。延长挡位可选 5°，10°，15°，20°，和 25° 屈曲挡位可选 30°，45°，60°，75° 和 90°。

*请在医生或专业人士指导下购买和使用。

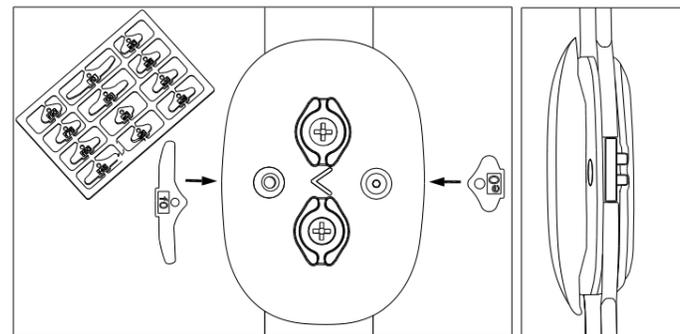

保养与维护

大身外套可以用中性洗涤剂和 30℃ 水手洗，并自然风干。切勿放入干衣机或使用其他热源进行干燥。

金属部分不可用水清洗，铰链可用干硅胶喷雾来润滑。

警告：如果您在使用此产品时感到疼痛，肿胀，感觉变化，或有不适的反应，请停止使用并联系您的医生。

仅适用于单例患者。

注意：该设备是只有一个元素的整体治疗方案由医疗专业人员管理，不能保证通过使用该装置可以防止损伤。

四. 产品基本环境

- 1) 环境温度：-15~60℃
- 2) 相对湿度：≤80%

五. 产品材料

- 1) 高弹力外套：氨纶纤维
- 2) 金属支架：铝合金/不锈钢
- 3) 搭扣：尼龙
- 4) 角度调整钥匙：尼龙/碳素钢
- 5) 绑带：尼龙/聚氨酯/聚酯

六. 禁忌症

- ⚠ 非稳定性骨折慎用；
- ⚠ 骨质疏松症慎用；
- ⚠ 认知缺陷慎用；
- ⚠ 骨质性关节强硬等慎用；

七. 产品的保管，运输及有效期

- 1) 产品有效期：5 年。
- 2) 产品的保管：未使用前请放置在干燥、清洁的室内，保证室内通气。
- 3) 运输：本产品在进行储存及运输的过程，应防尘、防潮、防污染。

八. 废弃物处理

包装纸（包装袋）的处理：本产品的包装请根据所属地区法例进行弃置处理，对垃圾进行分类。

九. 标记符号及图片说明

⚠ 注意，警告

🚫 禁止机洗

☀ 避免日晒

🚫 包装破损时切勿使用

🕒 有效期为 5 年

📖 参考使用说明

十. 配件清单

说明书----- 1 份
角度调整配件/螺丝----- 1 个（套）
角度调整钥匙----- 1 个
六角扳手----- 1 个
膝衬垫----- 1 个（套）

十一. 售后承诺

保修：所有产品从购买之日起为原始日期，正常磨损和撕裂的产品在使用过程中不被视为缺陷。

以下部件自购买之日起至质保期内，如果出现材料或工艺方面的缺陷，请直接联系你的销售商，简单医疗科技有限公司将对设备及附件进行完全或部分维修或更换。

金属支架----- 1 年

十二. 厂家信息

【产品名称】膝部固定器
【生产企业名称】东莞市雅创实业有限公司
【地址】广东省东莞市凤岗镇米亚路 1 号
【邮政编码】523696
【网址】www.acmould.com